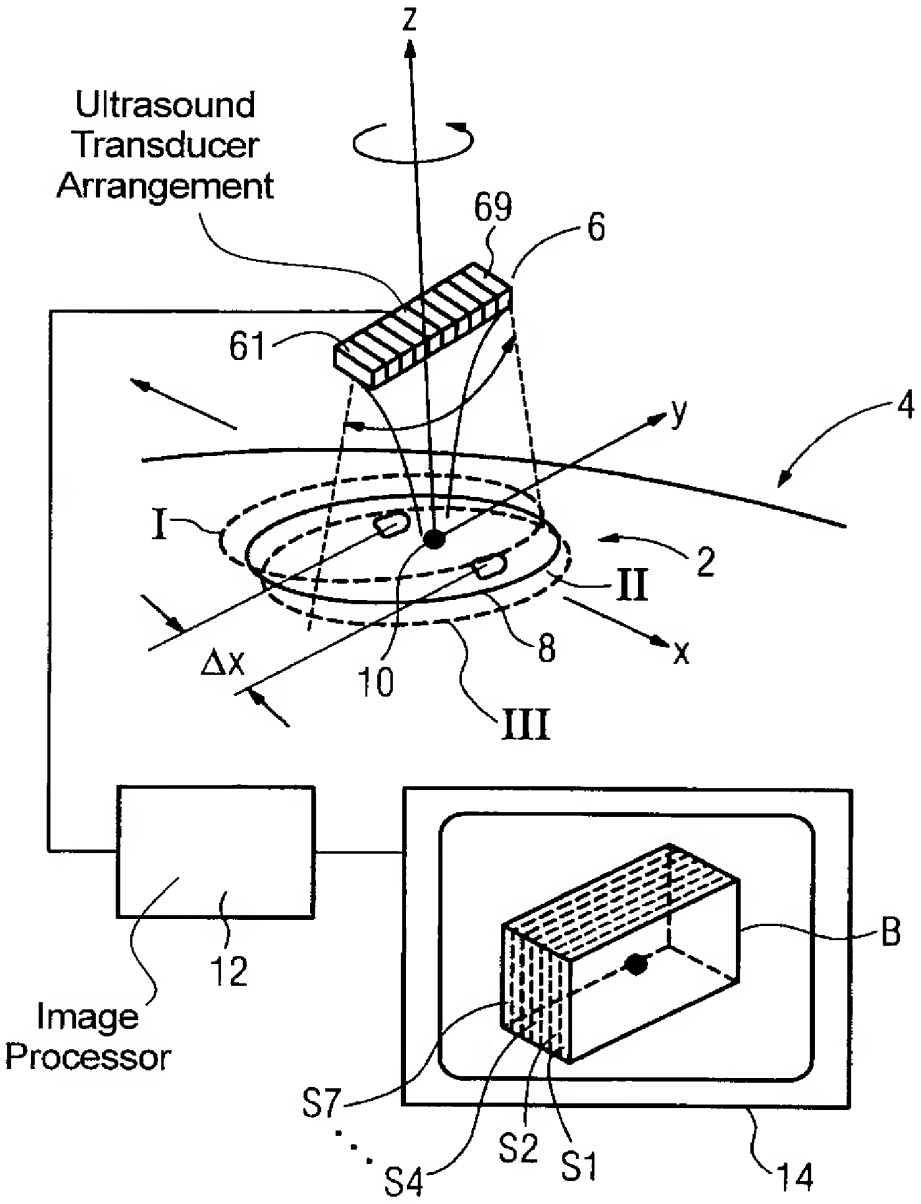
z
Ultrasound
Transducer
Arrangement
69
6
61
y
4
I
2
II
Δx
10
8
x
III
12
Image
Processor
B
S7
S4
S2
S1
14